




Medtronic

INFUSE[®] Bone Graft/ LT-CAGE[®] Device

Product Overview

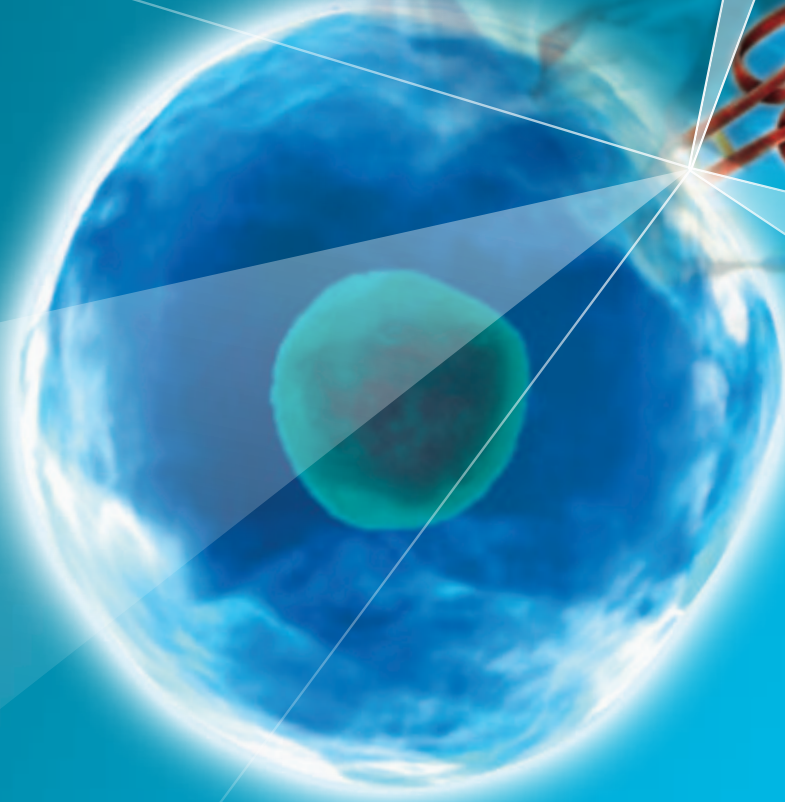

INFUSE® Bone Graft/LT-CAGE® Device

INFUSE® Bone Graft/LT-CAGE® Device Product Overview

Spine

Product Information

		INFUSE® Bone Graft/LT-CAGE® Device				
FDA-Approved Spine Indication		Single-level ALIF with Metallic Interbody Fusion Device from L2–S1				
Mechanism of Action (MOA)		High Osteoinduction				
Composition	Cells	Attracted by Chemotaxis				
	Carrier/Scaffold	Absorbable Collagen Sponge (ACS)				
	Signal	rhBMP-2				
rhBMP Concentration		1.5mg/cc				
Available Sizes		XX Small	X Small	Small	Medium	Large Large II
rhBMP Delivered		1.05mg	2.1mg	4.2mg	8.4mg	12mg
Graft Produced		0.7cc	1.4cc	2.8cc	5.6cc	8.0cc
List Price		\$876 to \$5,408				
Sterilization Method		Filter Sterilization Maintains Bioactivity Level				
FDA Regulatory Status		PMA Proven Safe and Clinically Effective				

Preclinical Data: Fusion Success

		rhBMP-2/ACS
Rabbit Pseudo Repair		100% (vs. 29% for ICBG) [†]
Sheep Interbody		100% (vs. 33% for ICBG) [†]

[†]Animal studies not necessarily indicative of human clinical outcomes.

Clinical Data

		INFUSE® Bone Graft/LT-CAGE® Device
Study Design		Single-level ALIF with LT-CAGE® Device
Total Patients in IDE Spine Study		277 rhBMP-2 Patients
Smokers Included in Study		32.9% of Patients
Fusion Assessment		X-ray and CT
Fusion Success at 24 Months		94.5% ¹
Fusion at Long-term Follow-up (Total)		98.5% at 6 Years (128/130) ²
Patients Working at 6-year Follow-up		68% (vs. 52% Preoperatively)

INFUSE® Bone Graft/LT-CAGE® Device

INFUSE® Bone Graft/LT-CAGE® Device Product Overview *continued*

FDA APPROVAL PATHWAYS

Pathway	Time to Market	Clinical Data Required	IRB Approval Required
IDE ⇨ PMA	Approximately 6 to 8 years	Large Pivotal Trial for Safety and Efficacy	No

IDE = Investigational Device Exemption
PMA = Pre-market Approval

PMA Explanation

- » Therapy is unique and represents a significant advancement in the treatment of a disease or condition
- » Must demonstrate safety and efficacy in a large pivotal clinical trial
- » IRB approval not required to use

References

1. Burkus JK, Gornet MF, Dickman CA, Zdeblick TA, Anterior lumbar interbody fusion using rhBMP-2 with tapered interbody cages. *J Spinal Discord Tech.* 2002 Oct;15(5):337-492.
2. Data on file.



BRIEF SUMMARY OF INDICATIONS, CONTRAINDICATIONS, AND WARNINGS FOR:

**INFUSE® BONE GRAFT/LT-CAGE® LUMBAR TAPERED FUSION DEVICE
INFUSE® BONE GRAFT/INTER FIX™ THREADED FUSION DEVICE
INFUSE® BONE GRAFT/INTER FIX™ RP THREADED FUSION DEVICE**

The INFUSE® Bone Graft/Medtronic Titanium Threaded Interbody Fusion Device is indicated for spinal fusion procedures in skeletally mature patients with degenerative disc disease (DDD) at one level from L2-S1, who may also have up to Grade I spondylolisthesis or Grade 1 retrolisthesis at the involved level. The INFUSE® Bone Graft/LT-CAGE® Lumbar Tapered Fusion Device is to be implanted via an anterior open or an anterior laparoscopic approach. INFUSE® Bone Graft with either the INTER FIX™ or INTER FIX™ RP Threaded Fusion Device is to be implanted via an anterior open approach.

The INFUSE® Bone Graft/Medtronic Titanium Threaded Interbody Fusion Device consists of two components containing three parts – a metallic spinal fusion cage, a recombinant human bone morphogenetic protein and a carrier/scaffold for the bone morphogenetic protein and resulting bone. These components **must** be used as a system for the prescribed indication described above. The bone morphogenetic protein solution component **must not** be used without the carrier/scaffold component or with a carrier/scaffold component different from the one described in this document. The INFUSE® Bone Graft component **must not** be used without the Medtronic Titanium Threaded Interbody Fusion Device component.

NOTE: The INTER FIX™ Threaded Fusion Device and the INTER FIX™ RP Threaded Fusion Device may be used together to treat a spinal level. LT-CAGE® Lumbar Tapered Fusion Device implants are not to be used in conjunction with either the INTER FIX™ or INTER FIX™ RP implants to treat a spinal level.

The INFUSE® Bone Graft/Medtronic Titanium Threaded Interbody Fusion Device is contraindicated for patients with a known hypersensitivity to recombinant human Bone Morphogenetic Protein-2, bovine Type I collagen or to other components of the formulation and should not be used in the vicinity of a resected or extant tumor; in patients with any active malignancy or patients undergoing treatment for a malignancy; in patients who are skeletally immature; in pregnant women; or in patients with an active infection at the operative site or with an allergy to titanium or titanium alloy.

There are no adequate and well-controlled studies in human pregnant women. In an experimental rabbit study, rhBMP-2 has been shown to elicit antibodies that are capable of crossing the placenta. Women of child bearing potential should be warned by their surgeon of potential risk to a fetus and informed of other possible orthopedic treatments. The safety and effectiveness of this device has not been established in nursing mothers. Women of child-bearing potential should be advised to not become pregnant for one year following treatment with this device.

Please see the package insert for the complete list of indications, warnings, precautions, adverse events, clinical results, definition of DDD, and other important medical information. The package insert also matches the sizes of those sized devices that are indicated for use with the appropriate INFUSE® Bone Graft kit.

CAUTION: Federal (USA) law restricts this device to sale by or on the order of a physician with appropriate training or experience.

**BRIEF SUMMARY OF INDICATIONS, CONTRAINDICATIONS, AND WARNINGS FOR:
INFUSE® BONE GRAFT**

INFUSE® Bone Graft is indicated for treating acute, open tibial shaft fractures that have been stabilized with IM nail fixation after appropriate wound management. INFUSE® Bone Graft must be applied within 14 days after the initial fracture. Prospective patients should be skeletally mature.

INFUSE® Bone Graft consists of two components – recombinant human Bone Morphogenetic Protein-2 solution and a carrier/scaffold for the bone morphogenetic protein solution and resulting bone. These components **must** be used as a system. The bone morphogenetic protein solution component **must not** be used without the carrier/scaffold component or with a carrier/scaffold component different from the one described in this document.

INFUSE® Bone Graft is contraindicated for patients with a known hypersensitivity to recombinant human Bone Morphogenetic Protein-2, bovine Type I collagen or to other components of the formulation and should not be used in the vicinity of a resected or extant tumor, in patients with an active malignancy or patients undergoing treatment for a malignancy. INFUSE® Bone Graft should also not be used in patients who are skeletally immature, in patients with an inadequate neurovascular status, in patients with compartment syndrome of the affected limb, in pregnant women, or in patients with an active infection at the operative site.

There are no adequate and well controlled studies in human pregnant women. In an experimental rabbit study, rhBMP-2 has been shown to elicit antibodies that are capable of crossing the placenta. Women of child bearing potential should be warned by their surgeon of potential risk to a fetus and informed of other possible orthopedic treatments. The safety and effectiveness of this device has not been established in nursing mothers. Women of child-bearing potential should be advised to not become pregnant for one year following treatment with this device.

Please see the package insert for the complete list of indications, warnings, precautions, adverse events, clinical results, and other important medical information.

CAUTION: Federal (USA) law restricts this device to sale by or on the order of a physician with appropriate training or experience.

**BRIEF SUMMARY OF INDICATIONS, CONTRAINDICATIONS, WARNINGS, AND PRECAUTION FOR:
INFUSE® BONE GRAFT FOR CERTAIN ORAL MAXILLOFACIAL AND DENTAL REGENERATIVE USES**

INFUSE® Bone Graft is indicated as an alternative to autogenous bone graft for sinus augmentations, and for localized alveolar ridge augmentations for defects associated with extraction sockets.

The INFUSE® Bone Graft consists of two components – recombinant human Bone Morphogenetic Protein-2 (rhBMP-2) placed on an absorbable collagen sponge (ACS). These components **must** be used as a system for the prescribed indication. The bone morphogenetic protein solution component **must not** be used without the carrier/scaffold component or with a carrier/scaffold component different from the one described in the package insert.

INFUSE® Bone Graft is contraindicated for patients with a known hypersensitivity to recombinant human Bone Morphogenetic Protein-2, bovine Type I collagen or to other components of the formulation and should not be used in the vicinity of a resected or extant tumor, in patients with any active malignancy or patients undergoing treatment for a malignancy, in pregnant women, or patients with an active infection at the operative site.

There are no adequate and well-controlled studies in human pregnant women. In an experimental rabbit study, rhBMP-2 has been shown to elicit antibodies that are capable of crossing the placenta. Women of child bearing potential should be warned by their surgeon of potential risk to a fetus and informed of other possible dental treatments. The safety and effectiveness of this device has not been established in nursing mothers. Women of child-bearing potential should be advised to not become pregnant for one year following treatment with this device.

INFUSE® Bone Graft has not been studied in patients who are skeletally immature (<18 years of age or no radiographic evidence of epiphyseal closure).

Please see the package insert for the complete list of indications, warnings, precautions, adverse events, clinical results, and other important medical information.

www.medtronic.com

Medtronic

Spinal and Biologics Business
Worldwide Headquarters

2600 Sofamor Danek Drive
Memphis, TN 38132

1800 Pyramid Place
Memphis, TN 38132

(901) 396-3133
(800) 876-3133
Customer Service: (800) 933-2635

For more information visit
www.myspinetools.com

